














Quick guide






rev.1 02/2020

Patient chair control

Control panel			
Backerest down As long as pressed (manual)		Backerest up As long as pressed (manual)	
Chair down As long as pressed (manual)		Chair up As long as pressed (manual)	
Chair to autoposition (automatic)		Chair rinsing/last position (automatic)	
Memory 1 (automatic)		Memory 2 (automatic)	
		Memory 3 (automatic)	
Locking Chair Movements		OK	Keep the key pressed for approx. 3 seconds until a beep is heard to lock the dental chair movements















Foot Control			
Backerest down As long as pressed (manual)		Backerest up As long as pressed (manual)	
Chair down As long as pressed (manual)		Chair up As long as pressed (manual)	

Dental unit control











Control panel		
Operating lamp		
Cup Fill	(Short activation)	
Bowl rinse	(Short activation)	
Door open / assistant call function		
Time /date settings		

Foot Control
Function can be programmed

Instrument control


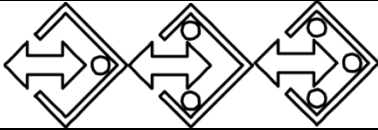


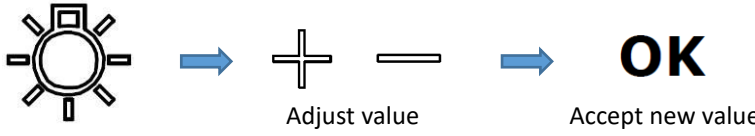





Control panel		
User profile	    	OK
	press until "CURRENT USER No." appears	Adjust value
Spray		Chip Blower Press level A
Clean Spray		
		Fiber optic light
		
Increase/decrease parameter (power, rpm, transmission ratio, torque, etc.)	 	Confirm parameter
		OK
Turbine		
Speed or fixed / progressive power control		
Scaler (Enabling the SCALER, PERIO AND ENDO functions depends on the installed scaler model.)		
Scaler function		Perio function
		
		Endo function
		

Instrument control

Control panel			
Micromotor			
Memory 1		Memory 2	
Memory 3		Speed or fixed / progressive power control	
			
Micromotor Brushless			
Memory 1		Memory 2	
Memory 3		Speed or fixed / progressive power control	
		(*)Fast mode	FAST
(*)Auto Forward mode	AUTO FORWARD	(*)Transmission Ratio	RATIO 1X
		(*)Maximum Torque	TORQUE
Reversing Rotation Direction Move the foot control lever A to the left and press it downwards until a beep is heard.			
Reversing Rotation Direction move the central lever A to the left until a beep is heard.			

(*) Only for enabled brushless micromotor

Programming

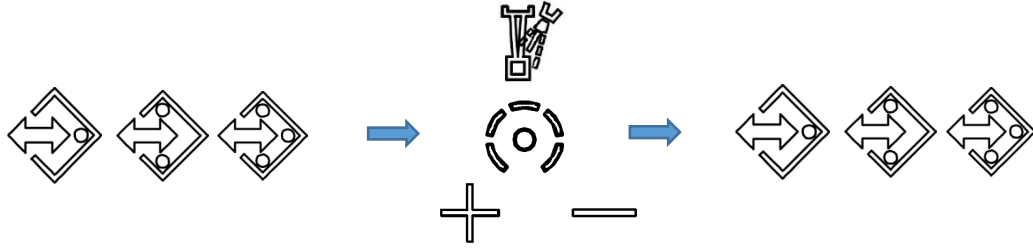Control panel	
User profile setting	
<p>User profile</p>  <p>press until "CURRENT USER No." appears Adjust value Accept new value</p>	
Patient chair settings	
<p>Memory 1-2-3 (automatic)</p> 	<p>To save a dental chair position, move the chair to the required position and hold down the key until you hear the beep that indicated the position is saved.</p>
<p>Chair to autoposition (automatic)</p> 	<p>To save a dental chair position, move the chair to the required position and hold down the key until you hear the beep that indicated the position is save. This enables storage of the pantographic arm reset position.</p>
<p>Chair rinsing (automatic)</p> 	<p>To save a dental chair position, move the chair to the required position and hold down the key until you hear the beep that indicated the position is save. This enables storage of the rinse position.</p>
Instrument settings	
<p>Instrument Lighting</p>  <p>Adjust value Accept new value</p>	<p>Spray</p> 
Cup filling and spitton rinsing time	
<p>Cup Fill</p>  <p>Press for 3 seconds and release the button when the desired level is reached in the cup.</p>	<p>Spittoon Rising</p>  <p>Press for 3 seconds and release the button when the desired rinsing time has elapsed.</p>
Micromotor settings	
<p>Memory 1-2-3</p>  <p>Select programs Adjust value Press for few seconds (beep)</p>	
Clock and data settings	
<p>Clock and data</p>  <p>Adjust value Accept new value</p>	