Quick guide

rev.0 01/2019

Patient chair control

Control panel

Backerest down **As long as pressed** (manual) 	**Backerest up** **As long as pressed** (manual) 
Chair down **As long as pressed** (manual) 	**Chair up** **As long as pressed** (manual)
Chair to autoposition (automatic) 	**Chair rinsing/last position** (automatic)

Memory 1 (automatic) 	**Memory 2** (automatic) 	**Memory 3** (automatic) 

Locking Chair Movements	Press the key for approx. 3 seconds until a beep is heard to disable the dental chair

Foot Control

Backerest down **As long as pressed** (manual)	**Backerest up** **As long as pressed** (manual)
Chair down **As long as pressed** (manual)	**Chair up** **As long as pressed** (manual)

Chair Platform

Recall the memory that was previously activated (automatic) 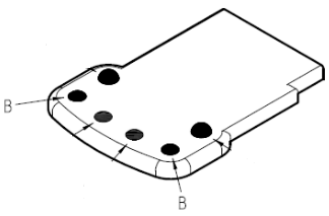	**Chair to autoposition** (automatic) 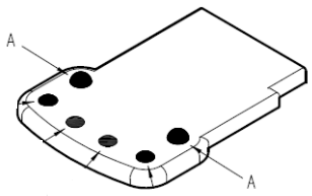
Chair rinsing/last position (automatic) 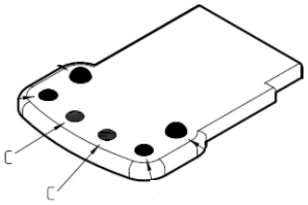	

Dental unit control

Control panel		
Operating lamp		
Cup Fill	(Short activation)	
Bowl rinse	(Short activation)	
Door open / assistant call function		
Time /date settings		

Foot Control
Function can be programmed

Instrument control

Control panel		
User profile		
press until “CURRENT USER No.” appears	Adjust value	Accept new value
Spray **Clean Spray**	**Chip Blower** **Press level A** 	**Fiber optic light**
Increase/decrease parameter (power, rpm, transmission ratio, torque, etc.) 		**Confirm parameter** **OK**
Turbine		
Speed or fixed / progressive power control 		
Scaler (Enabling the SCALER, PERIO AND ENDO functions depends on the installed scaler model.)		
Scaler function 	**Perio function** 	**Endo function** 

Instrument control

Control panel

Micromotor

Memory 1	**Memory 2**	**Memory 3**
Speed or fixed / progressive power control		

Micromotor Brushless

Memory 1	**Memory 2**	**Memory 3**
Speed or fixed / progressive power control	**(*)Fast mode** **FAST**	**(*)Auto Reverse mode** **AUTO REVERSE**
(*)Auto Forward mode **AUTO FORWARD**	**(*)Transmission Ratio** **RATIO 1X**	**(*)Maximum Torque** **TORQUE**

Reversing Rotation Direction
Move the foot control lever A to the left and press it downwards until a beep is heard.



Reversing Rotation Direction
move the central lever A to the left until a beep is heard.



(*) Only for enabled brushless micromotor

Programming

Control panel

User profile setting

User profile



press until “CURRENT USER No.” appears — Adjust value — Accept new value

Patient chair settings

Memory 1-2-3 (automatic)

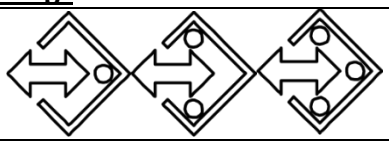

To save a dental chair position, move the chair to the required position and hold down the key until you hear the beep that indicates that the position has been saved.

Chair to autoposition (automatic)



To save a dental chair position, move the chair to the required position and hold down the key until you hear the beep that indicates that the position has been saved. This enables storage of the pantographic arm reset position.

Chair rinsing (automatic)

To save a dental chair position, move the chair to the required position and hold down the key until you hear the beep that indicates that the position has been saved. This enables storage of the rinse position.

Instrument settings

Instrument Lighting

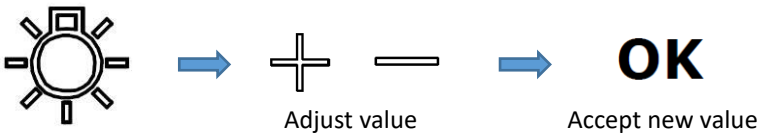

Adjust value — Accept new value

Spray

Cup filling and spitton rinsing time

Cup Fill

Press for 3 seconds and release the button when the desired level is reached in the cup.

Spittoon Rising



Press for 3 seconds and release the button when the desired rinsing time has elapsed.

Micromotor settings

Memory 1-2-3

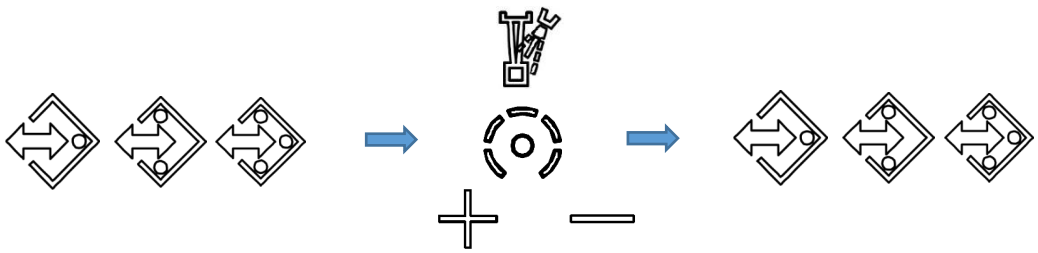

Select programs — Adjust value — Press for few seconds (beep)

Clock and data settings

Clock and data



Adjust value — Confirm new value